

# 

# the world's first neurophthalmoscope

8

exams in 12 minutes

- **ᡏ** Gaze holding
- **♂** Ocular Alignment
- **Solution** Fusional Amplitudes
- **Smooth Pursuit**
- *▼* Saccades
- **Visual Field**
- **⋘** Afferent Pupillary Function
- *▼* Efferent Pupillary Function

## neos

- **⋘** Increase patient comfort with a head-mounted device
- Margine of the state of the sta
- **⋘** Inspire greater precision with quantitative reporting

### Industry-leading eye tracking


neos uses infrared eye tracking that records eye movements at 200Hz, comfortably mounted in a headset that features active cooling to ensure patient comfort.

neos is compatible with contact lenses and includes a range of refractive error correction lens inserts.

### Data securely in the cloud

neos processes all data in the cloud, enabling you to easily access reports from your desk and attach them to your local electronic health record system.



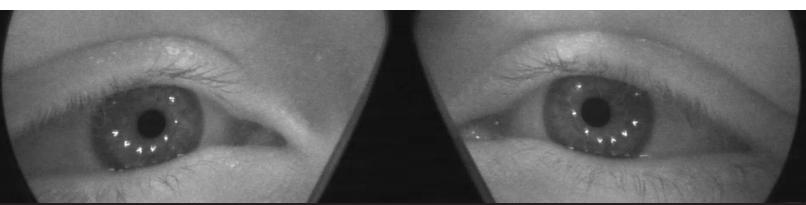



"My goal is to democratize specialist knowledge of neuroophthalmologists, enabling the earlier diagnosis of neurological disorders."

Dr. Mathias Abegg, MD, PhD Co-Founder and Medical Director machine **MD** 












### **Optimized stimuli**

Fixation and image clarity of a visual target require placement and maintenance of the fovea on the target<sup>1</sup>.

neos<sup>--</sup> presents a novel stimulus: an Unidentified Flying Object, UFO, projected at infinite distance (over 20m).

In addition to the neos report for gaze holding, stability of fixation is also interesting to review in the neos tests for smooth pursuit and during the fusional amplitude tests of convergence.

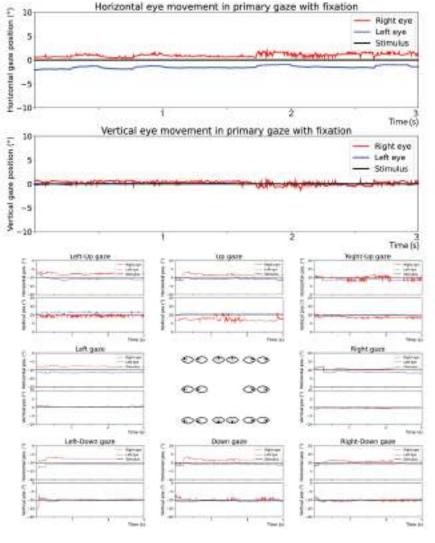

 $1.\,Rucker\,JC.\,Ny stagmus\,and\,Saccadic\,Intrusions.\,Contin\,Minneap\,Minn.\,2019; 25(5): 1376-1400.\,doi: 10.1212/CON.000000000000000772$ 



### **Automated alternate cover test**


The neos test sequence comprises alternate covers lasting 1.5 seconds each, beginning with primary gaze followed by the ±10° cardinal gaze positions.

### Presented in the style of the Hess Screen

In the neos report, black points represent the stimulus position for the fixating eye, and the red / blue points represent the median position of the covered eye.

### **Median latent deviation**


The difference between the black dot and the coloured dot is the median deviation of the phoria in that gaze direction.

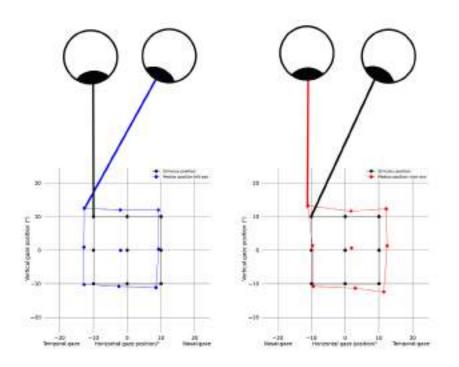

### Possible deviations include<sup>1</sup>:

- exodeviations, in which the eyes are turned laterally relative to one another
- esodeviations, in which the eyes are turned medially relative to one another
- hyperdeviations, in which one eye is higher than the other.

1. Rucker JC, et al. The neuro-ophthalmological examination. Handb Clin Neurol. 2011;102:71-94. doi:10.1016/B978-0-444-52903-9.00009-1

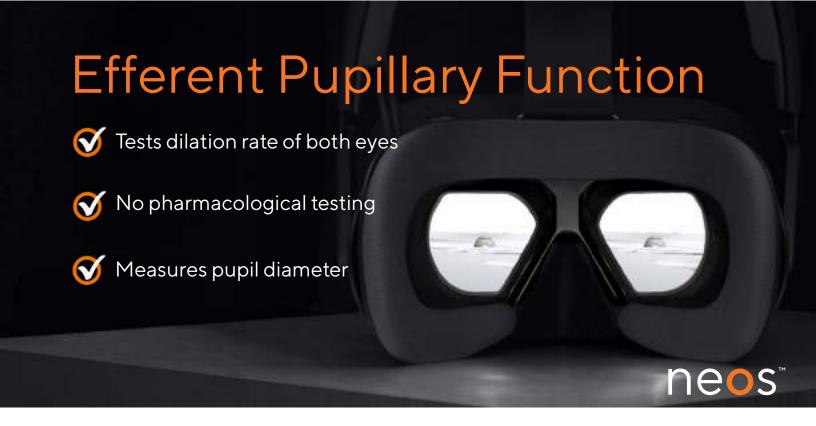


### Manual examinations miss 50% of anisocoria<sup>1</sup>

Pupil diameter and dynamics are determined by the interaction between the sympathetic and parasympathetic nervous systems. Whereas the parasympathetic system primarily drives pupillary constriction, the sympathetic system primarily drives pupillary dilation<sup>2</sup>.

Eyes observed via neos infrared cameras with bright screens:




Eyes observed via neos infrared cameras with dark screens:



neos presents a bright stimulus for 5 seconds, comprising an icy landscape with an igloo fixation point, projected at infinite distance (over 20m). neos then presents a dark screen with no fixation point for 15 seconds.

neos repeats this sequence 4 times, and the mean pupil diameter is highlighted for each eye in the below report.

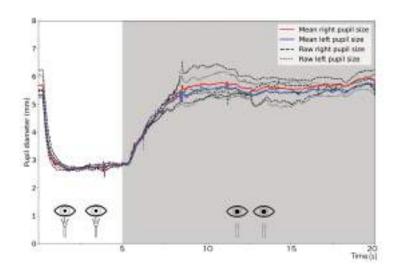

<sup>1.</sup> Couret D, et al. Reliability of standard pupillometry practice in neurocritical care: an observational, double-blinded study. Crit Care Lond Engl. 2016. Mar 13;20:99. doi: 10.1186/s13054-016-1239-z

<sup>2.</sup> Bower, M. M., et al. (2019). Quantitative Pupillometry in the Intensive Care Unit. Journal of Intensive Care Medicine. doi:10.1177/0885066619881124




# Only 40% of RAPD magnitudes are correctly estimated via manual swinging flashlight tests<sup>1</sup>.

Quantitative pupillometry can provide more reliable measurements with a lower error rate<sup>2</sup>. Pupillometry devices provide variables including maximum size, minimum size, constriction velocity, constriction amplitude, and response latency.

 neos" uses an automated, digitalized version of the swinging flashlight test: displaying a bright stimulus to one eye while the other eye is shown a dark screen for 3 seconds. The stimulus is repeatedly alternated between the two eyes.

neos plots minimum and maximum mean pupil diameters for each eye as black horizontal lines obtained during the test sequence.

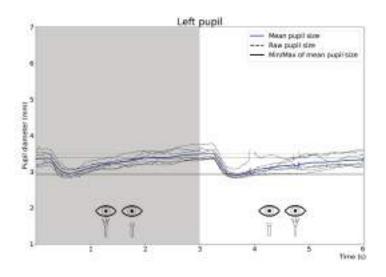


1. Boucher T, Fortin É, Evoy F. The standard swinging flashlight test: reliable or not (P1.9-009). Neurology. 2019; 92(15 Supplement): P1.9-009. 2. Bower MM, et al. Quantitative Pupillometry in the Intensive Care Unit. J Intensive Care Med. 2021;36(4):383-391. doi:10.1177/0885066619881124



neos" presents a forest scene with a fixation point of a fairy in a glowing circle, projected at infinite distance (over 20m). The stimulus is always shown under binocular conditions.

neos<sup>--</sup> measures gaze position while the patient tracks the fairy moving in the horizontal direction with two different velocities: 0.0625Hz followed by 0.125Hz. Two repetitions are made for each velocity with an amplitude of 15°.

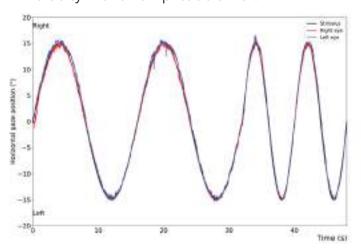

**Smooth-pursuit** movements allow clear vision of a moving target by holding the image steady on the fovea<sup>1</sup>. Pursuit performance requires focused attention to track a particular object.

**Saccades** are the fastest eye movements, with speeds as high as 700°/s and durations usually less than a tenth of a second. Their main function is to bring new images on to the fovea.

neos tests saccades by presenting the stimulus at ±10° and ±20° both horizontally and vertically. Each position is repeated several times and always binocularly.


neos measures gaze position relative to the stimulus, and also reports peak velocity for each eye at each angle (see right page).

Saccade related parameters include amplitude, saccadic latency, saccadic velocity, and saccadic accuracy<sup>2</sup>.

1. Kheradmand A, et al. Eye movements in vestibular disorders. Handb Clin Neurol. 2016;137:103-117. doi:10.1016/B978-0-444-63437-5.00008-X 2. Larrazabal AJ, et al. Video-oculography eye tracking clinical applications. Comput Biol Med. 2019;108:57-66. doi:10.1016/j.compbiomed.2019.03.025

# Horizontal & Vertical Saccades ✓ Prosaccadic eye movements ✓ Tests ±10° and ±20° ✓ Measures gaze position and peak velocity

neos

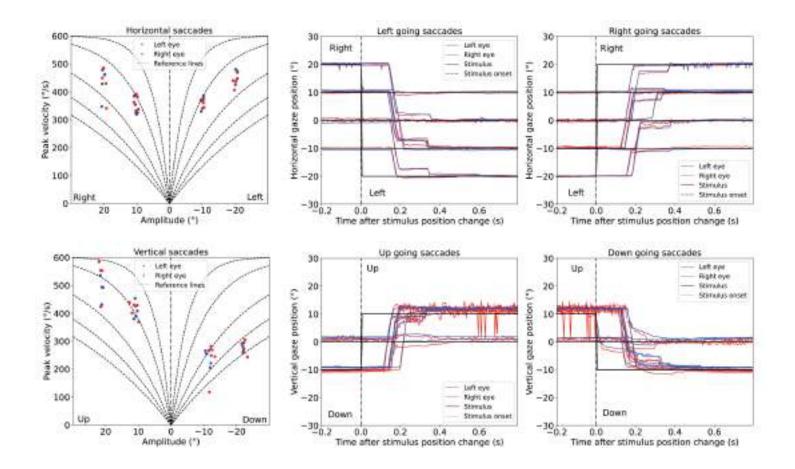


Peak velocity reference lines generated according to formulae in the book by Leigh RJ, Zee DS. The Neurology of Eye Movements.




neos<sup>--</sup> performs this test for both eyes using monocular stimuli. The patient is shown a fixation cross and a stimulus with maximal brightness appears according to an adaptive pattern. neos<sup>--</sup> detects the saccadic movement to the location of the stimulus and moves the fixation target accordingly.

### Visual Field Left Eye

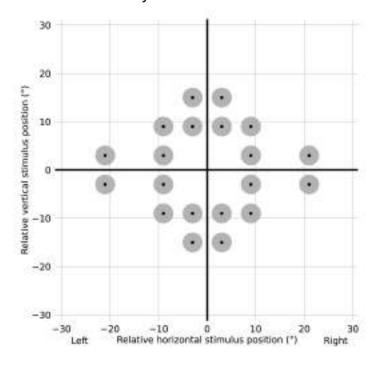


### Visual Field Right Eye

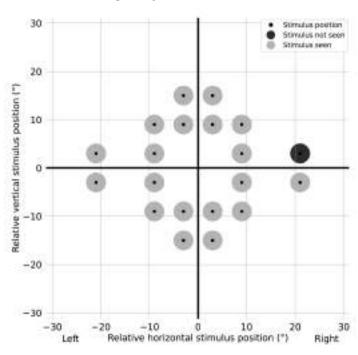





### Horizontal convergence: 7° (12 p.d.)

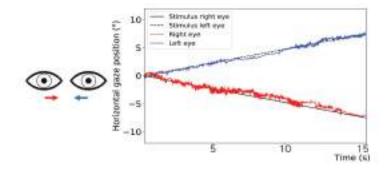

### Horizontal divergence: 7° (12 p.d.)

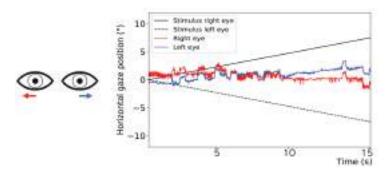

Vertical divergence, left  $\downarrow$ , right  $\uparrow$ : 3° (5 p.d.)

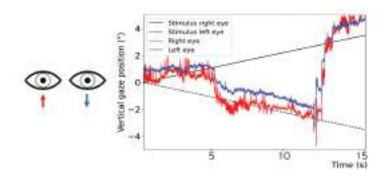

Vertical divergence, left ↑, right ↓: 3° (5 p.d.)

